

Periocular CO2 laser resurfacing: severe ocular complications from multiple unintentional laser impacts on the protective metal eye shields

Citation for published version (APA):

van Gemert, M. J. C., Bloemen, P. R., Wang, W.-Y., van der Geld, C. W. M., Nuijts, R. M. M. A., Hortoglu, H., Wolkerstorfer, A., de Bruin, D. M., van Leeuwen, T. G., Martino Neumann, H. A., & Jager, M. J. (2018). Periocular CO2 laser resurfacing: severe ocular complications from multiple unintentional laser impacts on the protective metal eye shields. *Lasers in Surgery and Medicine*, 50(10), 980-986.
<https://doi.org/10.1002/lsm.22951>

Document license:
TAVERNE

DOI:
[10.1002/lsm.22951](https://doi.org/10.1002/lsm.22951)

Document status and date:
Published: 01/12/2018

Document Version:
Publisher's PDF, also known as Version of Record (includes final page, issue and volume numbers)

Please check the document version of this publication:

- A submitted manuscript is the version of the article upon submission and before peer-review. There can be important differences between the submitted version and the official published version of record. People interested in the research are advised to contact the author for the final version of the publication, or visit the DOI to the publisher's website.
- The final author version and the galley proof are versions of the publication after peer review.
- The final published version features the final layout of the paper including the volume, issue and page numbers.

[Link to publication](#)

General rights

Copyright and moral rights for the publications made accessible in the public portal are retained by the authors and/or other copyright owners and it is a condition of accessing publications that users recognise and abide by the legal requirements associated with these rights.

- Users may download and print one copy of any publication from the public portal for the purpose of private study or research.
- You may not further distribute the material or use it for any profit-making activity or commercial gain
- You may freely distribute the URL identifying the publication in the public portal.

If the publication is distributed under the terms of Article 25fa of the Dutch Copyright Act, indicated by the "Taverne" license above, please follow below link for the End User Agreement:

www.tue.nl/taverne

Take down policy

If you believe that this document breaches copyright please contact us at:

openaccess@tue.nl

providing details and we will investigate your claim.

Periocular CO₂ Laser Resurfacing: Severe Ocular Complications From Multiple Unintentional Laser Impacts on the Protective Metal Eye Shields

Martin J. C. van Gemert, PhD,^{1*} Paul R. Bloemen, BSc,¹ Wei-Yong Wang, MD,² Cees W. M. van der Geld, PhD,³ Rudy M. M. A. Nuijts, MD, PhD,⁴ Hayri Hortoglu, MD,⁵ Albert Wolkerstorfer, MD, PhD,⁶ Daniel M. de Bruin, PhD,¹ Ton G. van Leeuwen, PhD,¹ H. A. Martino Neumann, MD, PhD,⁷ and Martine J. Jager, MD, PhD²

¹Department of Biomedical Engineering and Physics, Academic Medical Center, University of Amsterdam, Amsterdam, The Netherlands

²Department of Ophthalmology, Leiden University Medical Center, Leiden, The Netherlands

³Department of Chemistry, Eindhoven University of Technology, Eindhoven, The Netherlands

⁴Department of Ophthalmology, Maastricht University Medical Center, Maastricht, The Netherlands

⁵Amstelzijde Clinic, Amsterdam, The Netherlands

⁶Department of Dermatology, Academic Medical Center, University of Amsterdam, Amsterdam, The Netherlands

⁷Department of Dermatology, Erasmus Medical Center, Rotterdam, The Netherlands

Background and Objectives: A 36-year-old woman underwent CO₂ laser resurfacing for periocular rhytides using protective stainless steel Cox II ocular shields. Immediately after the treatment, corneal lesions were seen in both eyes. The left eye subsequently developed corneal ulceration and scarring, a deformed iris, cataract, and lower eye lashes showing signs of acute burns. The right cornea had a small inferior mid-peripheral superficial lesion and concomitant lower mid-peripheral burned eye lashes. Our objective was to determine the most likely cause of these ocular complications.

Study: We estimated temperature–time combinations that could induce corneal injury and cataract. Heat conduction effects from a heated cornea to the lens and from a heated ring of periocular skin to the cornea were computed. The temperature response of a shield following CO₂ laser irradiation was determined.

Results: We computed that cataract can develop when the corneal temperature reaches, for example, 80 °C for 14 seconds. A periocular ring of heated skin contributes little to the corneal temperature. After 7 pulses of consecutive CO₂ laser bursts in 7.5 seconds, the total shield area already reached a homogeneous temperature of 63 °C.

Conclusion: Despite uncertainties in procedural details and modeling of cataract temperatures, the eye injuries were caused beyond doubt by heating of tear-covered metal eye shields by at least 10 consecutive but unintentional laser impacts. *Lasers Surg. Med.* 50:980–986, 2018. © 2018 Wiley Periodicals, Inc.

Key words: CO₂ laser; periocular skin resurfacing; ocular complications; temperature–time predictions of cataract formation; corneal melting; burned eye lashes; metal eye shields

INTRODUCTION

Fractional carbon dioxide (CO₂) laser treatment has become a common procedure to treat various cutaneous conditions, including periocular rhytides. Sporadically, dermal side effects and complications occur [1] whereas very few publications address ocular complications [2–8]. We present a patient who was treated for periocular rhytides with a CO₂ laser. Immediately after the treatment, her vision was decreased and the eyes were irritated. Although both eyes had been protected by stainless steel Cox II shields, corneal clouding was seen in both eyes, with subsequent corneal melting and scarring in the left eye, with a deformed iris and the development of cataract. The lower eye lashes showed signs of acute burns. The right eye was less severely damaged.

Our objective was to determine whether heating of the metal eye shields by absorption of unintentional CO₂ laser impacts and/or heat conduction toward the cornea and the lens from a heated ring of periorbital skin by intentional CO₂ laser impacts could explain the complications.

Conflict of Interest Disclosures: All authors have completed and submitted the ICMJE Form for Disclosure of Potential Conflicts of Interest and none were reported.

Wei-Yong Wang is now at the Department of Ophthalmology, Haaglanden Medical Center, The Hague, The Netherlands.

Informed consent was obtained from the patient.

*Correspondence to: Martin J.C. van Gemert, PhD, Department of Biomedical Engineering and Physics, Academic Medical Center, University of Amsterdam, Meibergdreef 9, 1105 AZ Amsterdam, The Netherlands. E-mail: m.j.vangemert@amc.uva.nl

Accepted 26 May 2018

Published online 8 June 2018 in Wiley Online Library (wileyonlinelibrary.com).

DOI 10.1002/lsm.22951

Our second aim was to review the literature on this complication.

To achieve the first objective requires calculating (1) temperature–time combinations that result in (i) irreversible injury of the cornea and (ii) lens injury that leads to cataract; (2) temperature effects of heat conduction from (i) a hot cornea to the lens and (ii) a hot ring of periorbital skin to the cornea; And, measuring the temperature response of a Cox II eye shield to CO₂ laser impacts.

Challenging was that neither sufficient clinical details were available nor metal eye shield temperatures when hit by laser impacts, and that temperature histories of thermal lens cataract were unknown. This complication was handled by combining measured shield temperatures after laser impacts with analysis of existing cataract data and considering scenarios that comply with the clinical procedure.

MATERIALS AND METHOD

Calculating Heat Diffusion From a Hot Cornea to the Lens and From a Hot Ring of Periorbital Skin to the Center of the Cornea

For the thermal representation of an eye we used a sphere of water with a diameter of 2 cm and a thermal diffusivity of $1.5 \times 10^{-7} \text{ m}^2/\text{s}$, very close to the value of water ($1.43 \times 10^{-7} \text{ m}^2/\text{s}$) and the value often used for tissue ($1.77 \times 10^{-7} \text{ m}^2/\text{s}$ [9]). We assumed that the anterior surface of the lens is 2 mm away from the corneal surface. Because heating of the cornea occurred by a heated metal eye shield and/or by heat conduction from the heated periorbital skin, the temperature of the cornea is unknown. Therefore, we used the corneal temperature as a parameter that we varied between 60 and 100 °C. The initial lens temperature was 37 °C (Table 3 of ref. [10]). The temperature rise of the anterior lens capsule caused by heat conduction from the hot cornea follows by solving the bio-heat diffusion equation in this cornea-lens geometry using commercial package Comsol[®].

The effect of heat diffusion from a series of laser spots on the lower orbital rims was (over)estimated by taking a fully filled circumferential ring of periorbital skin that is instantaneously put at temperature levels between 60 and 100 °C, kept constant during 30 seconds; after that, the eye cooled down (Fig. 1). We used Comsol[®] again to calculate the temperature of the corneal center (Fig. 1). Because actual laser bursts are given consecutively and placed mainly on the lower rim, this approach obviously leads to overestimated temperatures compared to the original treatment. This approach was used for convenience to show (below) that even these exaggerated corneal and thus also lens temperatures are small.

Measured Temperature Response of a Cox II Eye Shield to CO₂ Laser Impacts

We measured the temperature response of a Cox II stainless steel eye shield at the concave side in response to CO₂ laser impacts on the convex side. First, freshly clotted blood was placed on the convex side of the metal shield to

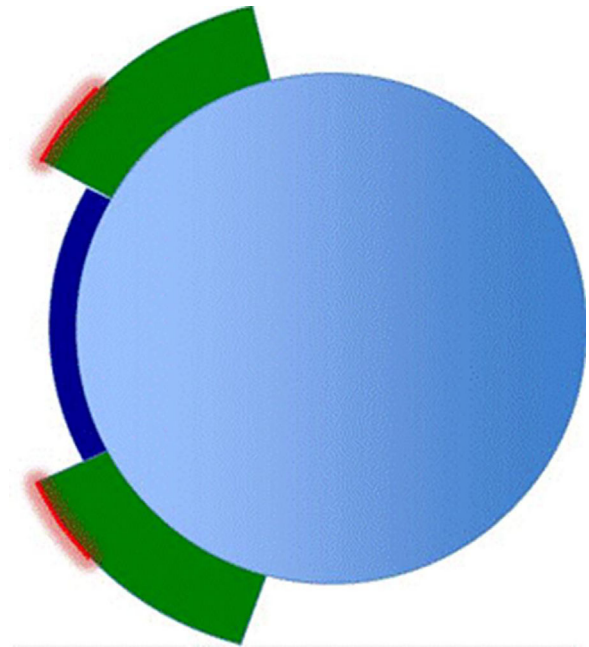


Fig. 1. Eye (blue sphere) with a ring-shaped skin layer of 3 mm thickness and 9 mm length around the orbital rim representing the periorbital skin (indicated in green), which was kept during the simulations at 60–100 °C during 30 s (indicated by a reddish line), and the metallic shield of 1 mm thickness in the middle area (dark blue layer).

mimic the absorption of laser impacts by the tear film that exists on the shield during actual treatment. Tear has a thermal diffusivity close to that of freshly clotted blood which is for 84% made up of water [11]. Second, we applied a honeycomb CO₂ laser pattern of 9 mm width and length, 1.3 mm spot diameter, 0.225 J per individual pulse, a pulse frequency during formation of the honeycomb pattern of 100 Hz, spot density 4 (i.e., 100% surface density of the laser spots), with a close to 1 Hz repetition frequency for consecutive honeycomb patterns. Third, we measured the temperature during and after multiple CO₂ laser impacts on the Cox II eye shield using a thermal camera (Seek Thermal, Comact XR). We included a black matted surface (Thorlabs BFP1) at the concave side of the metal to increase the emissivity of that surface. Finally, calibration was performed by testing at temperatures of 0 and 100 °C.

RESULTS

Clinical Case

A 36-year-old woman was treated with the UltraPulse CO₂ laser (Lumenis, Dreieich, Dreieichenhain, Germany) for periorbital rhytides at a cosmetic clinic according to a standard protocol. The patient was placed horizontally, and an anesthetic cream (lidocaine 23 mg/ml, tetracaine 3.5 mg/ml) was applied to the periorbital skin for 45 minutes. After removal of the cream, oxybuprocaine 0.4% eye drops and oculentum simplex ointment were applied to both eyes. Subsequently, stainless steel ocular shields (Type Cox II, size 25.5 × 22

× 1 mm, Oculo-Plastik Inc, Montréal, Québec) were placed, covering each eye, which caused distress to the patient. She was placed in a more supine position. For our analysis below it is essential that the eye lids under such circumstances never spontaneously close and hence do not cover the total area of the metal shield. The periocular skin was then treated with the laser in the Active FX mode using the CPG-scanning hand piece. The laser beam had a honeycomb pattern with an individual spot size of 1.3 mm, with energy per pulse of 0.1 J, frequency of 100 Hz and pulse duration of <1 milliseconds. For most of the procedure a spot density 3 (82% surface coverage of the individual pulses) was used and a spot density of 4 (100% coverage) for a row of second passes along the lower orbital rims.

During the procedure, which lasted 10–12 minutes, the patient did not indicate any problem. After removal of the eye shields, the patient indicated irritation and blurred vision in both eyes, which were consequently rinsed with sodium chloride 0.9% solution. Examination showed conjunctival hyperemia in both eyes and a white opacity of the left cornea. As her pain increased, she was immediately referred to the Ophthalmology Department (Leiden University Medical Center). At presentation, the best-corrected visual acuity was 0.6 (Snellen) in the right eye and 0.2 in the left eye (normal is about 1.0). The right cornea (Fig. 2a) showed grayish epithelium with a small inferior mid-peripheral superficial gray-white opacity with positive fluorescein staining. The left eye showed a superficial and deep intense white opaque cornea, positive

for fluorescein staining, with stromal edema, limbal ischemia, and a dilated pupil; the natural lens was not visible (Fig. 2b). Patient underwent superficial corneal debridement in both eyes, which failed in the left eye due to the rigidity of the superficial corneal layer. Both eyes were treated with dexamethasone-tobramycin ophthalmic ointment, cyclopentolate 1% eye drops, serum and cyclosporine eye drops, vitamin C tablets, and oral doxycycline. After 5 weeks, the right eye had recovered with a remaining minor midperipheral corneal opacity; visual acuity was 1.25. The left eye had a visual acuity of 0.02. Slit-lamp examination showed a persistent thickened cornea with a central epithelial defect, dilated pupil, deformed iris with a curled-up pupillary rim. The lens showed cataract with an anterior subcapsular star shape, a well-known ophthalmic characteristic of thermal damage. During the whole period, the eye pressure of both eyes remained within normal limits.

Two years later, she underwent cataract surgery on the left eye (Department of Ophthalmology, Maastricht). The final visual acuity at 35 months was 1.25 in the right eye, with a clear anterior segment, and 2/300 (hand motions at 2 m distance) in the left eye, with an intense white diffuse stromal scar with corneal vascularization and central stromal contraction and thinning, corneal flattening, a permanently curled-up pupillary rim and dilated pupil. For her left eye, she received a cosmetic contact lens with iris coloring. Seven years later (Fig. 2c and d), the only treatment of her left eye consists of tear substitutes (Fig. 2d).



Fig. 2. (a) Right eye, directly after treatment. Light burning of the lower middle lashes and perilimbal redness. (b) Left eye, directly after treatment. Severe burning of the lower eye lashes at the side of the nose and slight burning of all other lashes. The central cornea shows epithelial and stromal clouding. (c) Right eye seven years after treatment. (d) Left eye seven years after treatment. *N.B.* This patient has tattooed eyelines around both eyes.

Temperature–Time Combinations That Irreversibly Injure the Cornea and That Produce a Thermal Cataract

Assuming a normal corneal temperature (35 °C, [12]), Figure 3 shows the temperature–time behavior for corneal injury as measured in rabbit eyes [13]. Data from 181 humans [14–16] showed a similar corneal temperature of 34.8 °C and, although the size of the eyes and the eye lids are quite different, we have used Figure 3 as a reasonable approximation for human corneas.

In the literature, we found only two temperature histories that produced a cataract in rabbits (Fig. 2 of ref. [17]). Luckily, this allows deriving a generic temperature history of cataract formation by Arrhenius theory (Appendix A), with the results also shown in Figure 3.

Heat Diffusion Computations From the Hot Cornea to the Lens and From a Hot Ring of Periorbital Skin to the Center of the Cornea

A curled-up iris and the typical aspect of the anterior lens implied that a thermal cataract had developed. From Figure 3, the duration of the corneal temperature that predicts a cataract (open circles in Fig. 4) can be estimated. The computed anterior lens temperatures of cataract development in response to cornea temperatures of 60–100 °C are also shown in Figure 4. The corneal temperature–time combinations found are 60 °C–30 seconds; 67 °C–23 seconds; 70 °C–20 seconds; 80 °C–15 seconds; 90 °C–11 seconds; and 100 °C–10 seconds. The combination 67 °C–23 seconds will be used in the Discussion (Study limitations) to estimate the effects of using 0.1 J per pulse instead of 0.225 J.

The computed temperature increase at the center of the cornea in response to an instantaneous hot ring of periorbital skin, of 3 mm thickness (Fig. 1), with exposure to temperatures between 60 and 100 °C during 30 seconds and cooling thereafter, varied between 4.4 and 11.5 °C. As stated earlier, these corneal temperature effects overestimate the actual behaviors since laser bursts are given consecutively and mainly on the lower rim. Therefore, periorbital laser impacts along the lower rim cause a few degrees increased corneal temperature only, hardly affecting the anterior lens temperature.

Measured Temperature Response of a Cox II Eye Shield to CO₂ Laser Impacts

The presence of a tear film on the metal shield is an essential aspect of this laser treatment, because CO₂ laser light significantly absorbs in water. Local irritation and oxybuprocaine eye drops will stimulate tearing and the formation of a tear film. Therefore, experiments have been conducted with blood clotted on the metal shield; blood mimics the water film and is obviously easier to handle. Figure 5 shows the measured temperatures of a Cox II eye shield in response to 19 CO₂ laser honeycomb impacts (“plus” signs on the horizontal axis). First, we used a sterile Cox II eye shield. Second, we added blood drops to the convex part of the shield, waited 1 minute until the drops were clotted, and

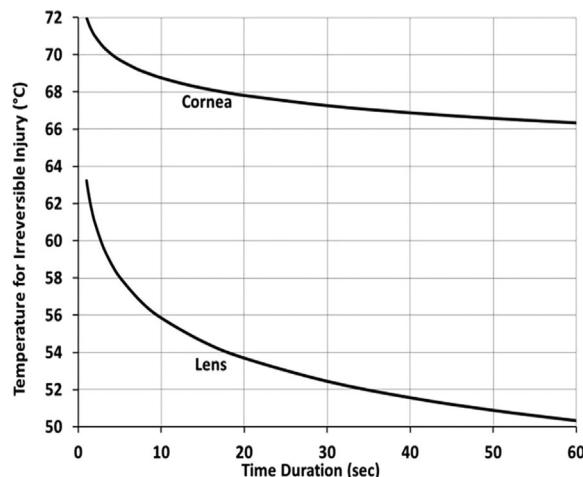


Fig. 3. Temperature–time duration curves derived from rabbit experiments that predict irreversible thermal corneal injury, using 35 °C as normal corneal temperature [10] (upper curve), and a thermal cataract, Equation (1) (lower curve).

irradiated the eye shield area with the clotted blood on its surface. As blood contains about 84% of water [11], we estimated the temperature response to 19 laser bursts of the eye shield with water (representing a tear film), by multiplying the data with clotted blood by 1/0.84 = 1.19. After 7 pulses in 7.5 seconds, the total shield area already reached 63 °C. Subsequently, the shield area retained a uniform temperature, also during cooling (137 seconds).

DISCUSSION

Most Likely Scenario That Caused the Corneal Injuries

We questioned how 10–20 consecutive CO₂ laser pulses could have had such an impact on the left eye. The pulses were part of a normal procedure and we hypothesized that the second pass on the left lower orbital rim had a more upward directed CO₂ laser hand piece, perhaps because the patient’s head was directed slightly more upward than normal, and that every CO₂ laser burst impacted on the eye shield. The exceedingly large absorbance of CO₂ laser light by tear-covered stainless steel would have caused a significant temperature rise of the metal shield. The shield’s excellent thermal properties would lead to spreading of the heated area over the total metal (and thus corneal) surface within 7.5 seconds (Fig. 5, dashed line “% Heated Area”). This hypothesis implies that the lower eye lashes should be burned. Because examination of the eyelids showed that this was indeed the case (Figs. 2a and b), we believe that placement of multiple unintentional CO₂ laser impacts on the metal eye shields is the most likely scenario that caused the ocular complications in this patient. Heat conduction from the hot cornea also heated up and injured the iris and caused a cataract. We emphasize that intraocular damage following this CO₂ laser procedure has not been described before.

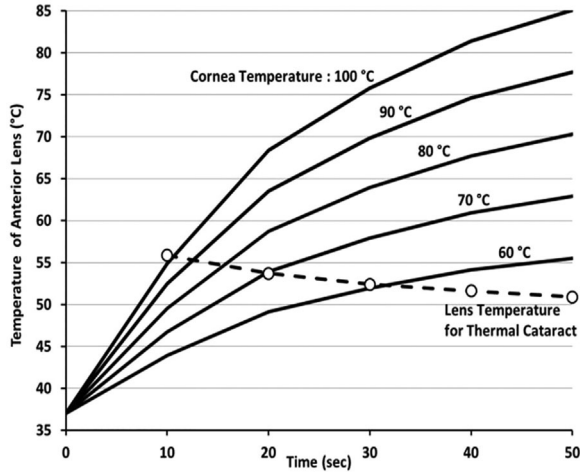


Fig. 4. Temperature of the anterior lens, at 2 mm inside the eye, assumed at 37 °C, as a function of the time of heat conduction duration for several corneal temperatures (60 °C to 100 °C). The temperature–time points that will predict the development of a cataract are indicated as circles.

This paper must create awareness for all physicians who perform periorcular CO₂ laser resurfacing procedures that unintentional CO₂ laser irradiation of metal eye shields, despite protecting the cornea against direct laser impact, has the capability of significantly heating up these shields (see, e.g., [18]). This effect is even intensified by the tear film (Fig. 5), a mechanism that has not been described before.

Study Limitations

Unfortunately, actual treatment details are unknown, for example, whether the second pass around the left lower orbital rim occurred immediately after the first pass and whether the first pass of laser bursts also hit the eye shield. If that were the case, the second pass would have started with an already increased shield temperature. For simplicity, we assumed that the first pass laser bursts missed the eye shield.

The way we modeled laser impacts on the periorbital skin led to overestimated responses. Since the resulting temperature rises were found to be negligible, the extent of overestimation is irrelevant. Also, the Arrhenius parameters for thermal cataract formation from only two experimental temperature–time combinations (Appendix A) have limited accuracy. However, the derived temperature–time curve (Fig. 3) is the only one available to date that describes cataract formation from an increased lens temperature. The outcome, that these cataract-causing temperatures are below those of corneal damage temperatures suggest that the prediction is meaningful; the opposite would have contradicted the observed damage events.

Cooling of the metal eye shield held in air (Fig. 5) is (much) faster than in the clinical situation, placed on the eye ball and intermittent layer of oculentum simplex,

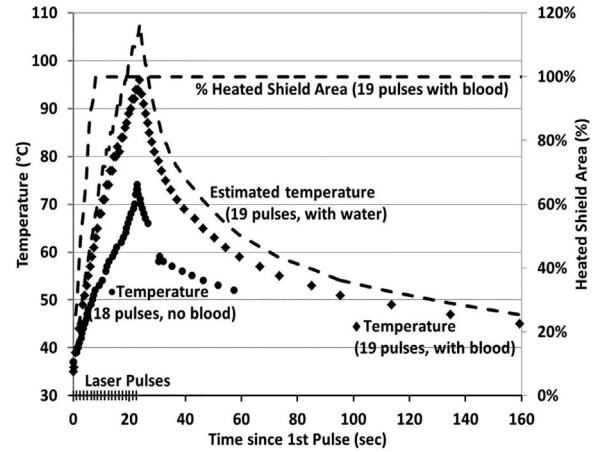


Fig. 5. Measured temperatures during heating and cooling of the Cox II shield in air in response to 19 CO₂ laser bursts (black lozenges) at 0.225 Joule, about 1 Hz per burst, 1.3 mm spot diameter, 9 mm width/length honeycomb pattern, about 100 Hz for individual pulses. Time points of the bursts are indicated by “plus” signs on the horizontal axis. At the right side (black dashed line, “% Heated Shield Area (19 pulses with blood)”, we plotted the area of the shield (in %) with an increased temperature. Also shown are measurements without added blood (black circles), and the computed estimated curve of the eye shield with water added (thick black dashed line), assuming whole blood contains 84% of water [11].

which has isolating properties (a 2.5 times smaller thermal diffusivity, Appendix B). Thus, it takes quite a long time before a temperature rise of the cornea has diffused away, contributing to corneal thermal damage and cataract formation at sufficiently high temperatures (Figs. 3 and 4).

The CO₂ experimental laser parameters (0.225 J) differed from those used clinically (0.1 J). However, the estimated temperatures of the Cox II shield with added water (Fig. 5) in response to 0.225 J laser pulses, can be easily transformed into temperatures from 0.1 J pulses by dividing temperature increase by 2.25. After 19 pulses, this would give a temperature of about 67 °C instead of 107 °C. Then, 70 °C would have been reached after 24.5 seconds, thus after 21 pulses. However, a longer time duration also lowers the critical temperature for corneal injury and cataract formation (Fig. 3). From Figure 4, one can see that development of a cataract occurs when the cornea temperature is about 67 °C during about 23 seconds.

Incidence of This Complication

This thermal complication either seems to be extremely rare or has been underreported in the literature as we found only five papers on this subject. In three, the authors described the thermal cause [2], one written in Korean [6], the third [3] gave a 0.3% incidence of corneal injury after CO₂ laser blepharoplasty, however, without details. In the other two [5,8], we believe the cause was thermal but the authors proposed other mechanisms.

Other Possible Causes

The review by Blanco et al. [4] did not refer to Widder et al. [2] and Christian et al. [5] but included many other mechanisms. Chemical damage can occur when the cream to anesthetize periorbital skin reaches the cornea, or when corneal eye shields are cleansed with chlorhexidine prior to insertion [5]. Thermally burned eye lashes, eyelid skin, and eyebrow hair have been described in a patient who was wearing mascara while cautery was applied to her eyelid lesion after excision [7]. Although our patient has tattooed eyeliner (Fig. 2), these lines were not damaged.

CONCLUSION

Despite uncertainties concerning procedural and cataract modeling details, our experiments on the Cox II shield (Fig. 5), the burned lower eye lashes (Fig. 2a and b), and the supporting heat diffusion computations have shown beyond doubt that consecutive CO₂ laser impacts hit both eye shields caused the left total shield area to reach a high temperature, probably over 70 °C, followed by a slow cooling rate. Heat conduction (Fig. 4) caused curling-up of the iris and a thermal cataract. The right shield also received CO₂ laser impacts but less than the left shield and only around the central part of the eye, shown by mid-peripheral corneal damage and burned lower middle eye lashes.

Few treatment options exist for thermal ocular injury. Our case thus emphasizes the importance of knowing the pitfalls of periocular CO₂ laser resurfacing procedures and, especially now that fractional CO₂ laser resurfacing is gaining in popularity, suggests adapting the safety guidelines with respect to the use of metal eye shields. Particularly, the eye shields should not only be positioned properly but the position of the CO₂ laser beam, visible by the pilot beam, should also be cautiously monitored as long as the laser is switched on.

REFERENCES

1. Alster TS, Lupton JR. Prevention and treatment of side effects and complications of cutaneous laser resurfacing. *Plast Reconstr Surg* 2002;109:308–316.
2. Widder RA, Severin M, Kirchhof B, Krieglstein GK. Corneal injury after carbon dioxide laser resurfacing. *Am J Ophthalmol* 1998;125:392–394.
3. Apfelberg DB. Summary of the 1997 ASAPS/ASPRS Laser Task Force Survey on Laser Resurfacing and Laser Blepharoplasty. *Plast Reconstr Surg* 1998;101:511–518.
4. Blanco G, Clavero A, Soparkar CNS, Patrinely JR. Periocular laser complications. *Semin Plast Surg* 2007;21:74–79.
5. Christian MM, Cox DO, Smith CV, Onouye T, Moy RL. Ocular damage due to chlorhexidine versus eyeshield thermal injury. *Dermatol Surg* 2001;27:153–157.
6. Kim JH, Ahn MW, Lee JS. Corneal burn caused by Carbon Dioxide Ultrapulsed laser for nevus removal. *J Korean Ophthalmol Soc* 2014;55:1376–1379.
7. Al Raqqad N, Liu C. Mascara: a cause of thermal burn after cautery for eye lid lesion excision; a case report. *J Clin Experiment Ophthalmol* 2010;1:105.
8. Litzinger TC, Vastine D. Bilateral corneal opacities in a LASIK patient after the use of titanium eyeshields. *J Cataract Refract Surg* 2011;37:1160–1164.
9. van Gemert MJC, Welch AJ. Approximate solutions for heat conduction: Time constants. In: Welch AJ, van Gemert MJC, editors. *Optical-Thermal response of laser-irradiated tissue*, Chapter 13. New York: Plenum Press; 1995. p 425.
10. Rahman A, Al-Ghadyan A, Cotlier E. Rise in temperature on exposure to sunlight or high ambient temperature. *Br J Ophthalmol* 1986;70:421–426.
11. Wahl HG. How accurately do we measure blood glucose levels in intensive care units (ICU) patients? *Best Practice Res Clin Anaesthesiol* 2009;23:387–400.
12. Mikesell GW. Corneal temperatures—A study of normal and laser injured corneas in the Dutch Belted Rabbit. *Am J Ophthalmol* 1978;55:108–115.
13. Barger CB, Deters OJ, Farrell RA, McCally RL. Epithelial damage in rabbit corneas exposed to CO₂ laser radiation. *Health Phys* 1989;56:85–95.
14. Mapstone R. Measurement of corneal temperature. *Exp Eye Res* 1968;7:237–243.
15. Fabiani C, Li Voti R, Rusciano D, Mutolo MG, Pescosolido N. Relationship between corneal temperature and intraocular pressure in healthy individuals: A clinical thermographic analysis. *J Ophthalmol* 2016;2016:3076031. <https://doi.org/10.1155/2016/3076031>
16. Giannaccare G, Fresina M, Agnifili L, Versura P. Ocular-surface temperature modification by cataract surgery. *J Cataract Refract Surg* 2016;42:983–989.
17. Kramar PO, Emery AF, Guy AW, Lin JC. The ocular effects of microwaves on hypothermic rabbits: A study of microwave cataractogenic mechanisms. *Ann NY Acad Sci* 1975;247:155–165.
18. Ries WR, Clymer MA, Reinisch L. Laser safety features of eye shields. *Lasers Surg Med* 1996;18:309–315.
19. Thomsen S, Pearce JA. Thermal damage and rate processes in biological tissues. In: Welch AJ, van Gemert MJC, editors. *Optical-thermal response of laser-irradiated tissue*. 2nd Edition. Dordrecht: Springer; 2011. Chapter 13. pp 487–549.

APPENDIX A. ARRHENIUS THEORY OF CATARACT FORMATION

We combined the two temperature–time ($T - \tau$) combinations that produced a cataract in rabbits (Fig. 2 of ref. [17]): 43.5 °C during 10 minutes and 41.5 °C during 20 minutes with Arrhenius kinetic rate theory ([19], Eq. 13.42), using

$$\ln(\tau) = \frac{E/R}{T} - \ln(A) \quad (1)$$

E is activation energy [J/mole], R the universal gas constant [8.3143 J/mole/K], T the temperature in Kelvin (0 °C is 273.15 K), and A the frequency factor [s^{-1}]. From the two data points the two unknowns in Equation (1) follow as $E/R = 34,530.5$ K and $\ln(A) = 102.65$. The ($T - \tau$) curve for a cataract is also given in Figure 3 (lower curve).

APPENDIX B. THERMAL DIFFUSIVITY OF OCULENTUM SIMPLEX

We used the available chemical composition and thermal data of the components, that is, 40% paraffin (thermal conductivity $k = 0.25$ W/m/°C, thermal diffusivity $\alpha = 0.081 \times 10^{-6}$ m²/s), 51.5% vaseline (α not found, $k = 0.18$ W/m/°C), 6% lanoline ($\alpha = 0.053 \times 10^{-6}$ m²/s), and 2.5% cetostearyl alcohol (here we used glycerol, $\alpha = 0.01 \times 10^{-6}$ m²/s). Assuming that α is proportional to k (implying identical product of density and heat capacity) gives $\alpha = 0.064 \times 10^{-6}$ m²/s for vaseline. Then, based on the composition, an estimated thermal diffusivity of oculentum simplex is $\alpha \approx (0.4 \times 0.081 + 0.515 \times 0.064 + 0.06 \times 0.053 + 0.025 \times 0.143) \times 10^{-6} = 0.07 \times 10^{-6}$ m²/s. Tissue has about 0.18×10^{-6} m²/s thus oculentum simplex has about a 2.5 times lower thermal diffusivity than tissue.