

Adaptive pressure control applied to mechanically ventilated patients

Citation for published version (APA):

Reinders, J., Hunnekens, B., Oomen, T., & van de Wouw, N. (2019). Adaptive pressure control applied to mechanically ventilated patients. In P. Patrinos, I. Markovsky, W. Michiels, J. Swevers, & S. Waldherr (Eds.), *Book of abstracts 38th Benelux Meeting on Systems and Control* (pp. 134). Katholieke Universiteit Leuven.

Document status and date:

Published: 01/01/2019

Document Version:

Publisher's PDF, also known as Version of Record (includes final page, issue and volume numbers)

Please check the document version of this publication:

- A submitted manuscript is the version of the article upon submission and before peer-review. There can be important differences between the submitted version and the official published version of record. People interested in the research are advised to contact the author for the final version of the publication, or visit the DOI to the publisher's website.
- The final author version and the galley proof are versions of the publication after peer review.
- The final published version features the final layout of the paper including the volume, issue and page numbers.

[Link to publication](#)

General rights

Copyright and moral rights for the publications made accessible in the public portal are retained by the authors and/or other copyright owners and it is a condition of accessing publications that users recognise and abide by the legal requirements associated with these rights.

- Users may download and print one copy of any publication from the public portal for the purpose of private study or research.
- You may not further distribute the material or use it for any profit-making activity or commercial gain
- You may freely distribute the URL identifying the publication in the public portal.

If the publication is distributed under the terms of Article 25fa of the Dutch Copyright Act, indicated by the "Taverne" license above, please follow below link for the End User Agreement:

www.tue.nl/taverne

Take down policy

If you believe that this document breaches copyright please contact us at:

openaccess@tue.nl

providing details and we will investigate your claim.

Adaptive pressure control applied to mechanically ventilated patients

Joey Reinders^{1,2}, Bram Hunnekens², Tom Oomen¹, and Nathan van de Wouw^{1,3}

1 Department of Mechanical Engineering, Eindhoven University of Technology, Eindhoven
2 DEMCON, Best

3 Department of Civil, Environmental & Geo-Engineering, University of Minnesota, U.S.A.
Email: j.m.f.reinders@tue.nl

Mechanical ventilation

Mechanical ventilation is used in Intensive Care Units (ICUs) to save lives of patients unable to breath on their own. Mechanical ventilation supports patients by ensuring adequate oxygenation and carbon dioxide elimination [1]. A schematic representation of a blower-driven mechanical ventilator attached to a patient is depicted in Figure 1. The system consists of a blower generating flow and pressure profiles, the hose-filter system, and the patient.

Relevant control problem

The control goal is to achieve accurate tracking of the patient airway pressure p_{aw} , i.e., $e = p_{target} - p_{aw}$ should be small with p_{target} the desired airway pressure. In commercial systems, unit feedforward with a linear feedback controller is used to achieve adequate tracking performance of p_{aw} . The feedback controller has to compensate for the pressure drop over the hose $\Delta p = p_{aw} - p_{out} = R_{lin}Q_{out}$. Moreover, the feedback controller is designed to ensure stability for a wide variety of patients, hence, performance is far from optimal. Predicting this pressure drop a priori is challenging, since it depends on several unknown factors:

- the patient, i.e., lung and airway, that is ventilated;
- the characteristics of the hose-filter system;
- (un)intended leakage in the system;
- spontaneous breathing activity of the patient.

Therefore, a controller is desired that accurately compensates for this pressure drop, and achieves accurate tracking of p_{target} . This controller should fulfill the following requirements:

- improve tracking performance, independent of the described unknown factors;
- handle time-varying system parameters;
- prevent overshoot in patient flow and therewith false ventilator induced triggered breaths;
- avoid using direct feedback on the patient airway pressure, p_{aw} sensor might come loose in practice.

Control approach

To improve tracking performance, an adaptive control approach is developed that compensates for the pressure drop Δp over the hose. This control approach uses the measured flow Q_{out} , and pressures p_{aw} and p_{out} to estimate the linear resistance of the hose R_{lin} . A recursive least squares algorithm is developed, see [2], to obtain the linear resistance

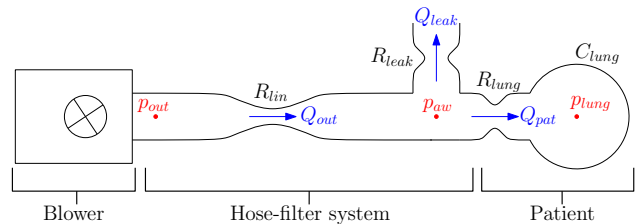


Figure 1: Schematic overview of the blower-hose-patient system.

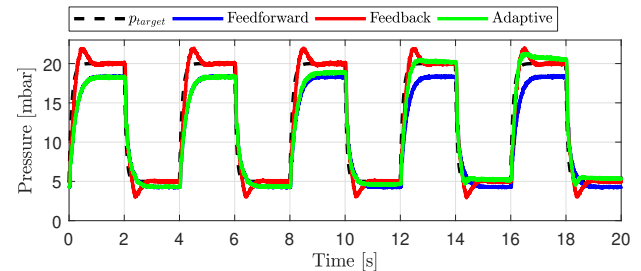


Figure 2: Experimental results comparing different control approaches.

estimate \hat{R}_{lin} . Using the estimate \hat{R}_{lin} and the measured flow Q_{out} , an estimate of the pressure drop $\Delta \hat{p} = \hat{R}_{lin}Q_{out}$ is used to compensate for the actual pressure drop. A stability result is derived that shows exact tracking of a time-varying reference, whilst ensuring all requirements and handling the unknown factors.

Experimental results

Through an experimental case study the improved tracking performance is shown, see Figure 2. The figure shows an improvement in tracking performance compared to feedback control, specifically, the undershoot has decreased. This improvement prevents overshoot in the patient flow Q_{pat} , improving patient comfort and consistency of treatment.

Further improvements could be achieved by considering a quadratic resistance model and/or the delays in the system in the scope of controller design.

References

- [1] M.A. Warner and B. Patel, "Mechanical Ventilation", in *Benumof and Hagberg's Airway Management*. Elsevier, 2013, pp. 981-997.
- [2] J. Reinders, F. Heck, B. Hunnekens, T. Oomen, and N. van de Wouw, "Online hose calibration for pressure control in mechanical ventilation," in *IEEE Proc. of the American Control Conference (ACC)*, 2019. (Accepted)